

# Methods for analysis and testing of coal and coke —

## Part 106: Ultimate analysis of coal and coke —

### Section 106.7 Determination of carbonate carbon content

ICS 75.160.10

## National foreword

This British Standard is the UK implementation of ISO 925:1997. BS 1016-106.7 will form a revision of Parts 6 to 11 of BS 1016. This section supersedes clauses **5** and **9** and **11** those parts of clause **11** relating to carbon (carbonate) as carbon dioxide in BS 1016-6.

The UK participation in its preparation was entrusted to Technical Committee SFI/3, Analysis and testing of coal and coke, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep the UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

Under a scheme for the rationalizing and restructuring of BS 1016, the parts numbered from 1 to 21 are being gradually withdrawn and replaced with parts in a new series. The full list of parts in the new series, together with the corresponding numbering of the old series and related ISO standards is given in BS 1016-100 *General introduction and sampling report*.

A list of organizations represented on this committee can be obtained on request to its secretary.

### Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the BSI Standards Catalogue under the section entitled “International Standards Correspondence Index”, or by using the “Find” facility of the BSI Standards Electronic Catalogue.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

**Compliance with a British Standard does not of itself confer immunity from legal obligations.**

### Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, the ISO title page, pages ii to iv, pages 1 to 4, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

### Amendments issued since publication

| Amd. No. | Date | Comments |
|----------|------|----------|
|          |      |          |
|          |      |          |
|          |      |          |
|          |      |          |
|          |      |          |

This British Standard, having been prepared under the direction of the Sector Board for Materials and Chemicals, was published under the authority of the Standards Board and comes into effect on 15 September 1997

© BSI 09-1999

ISBN 0 580 28416 6

# Contents

|                   | Page               |
|-------------------|--------------------|
| National foreword | Inside front cover |
| Foreword          | iii                |
| Text of ISO 925   | 1                  |

Licensed copy: Lee Chau Kee Library, HKUST, Version correct as of 03/01/2015, (c) The British Standards Institution 2013



INTERNATIONAL  
STANDARD

ISO  
925

Third edition  
1997-05-01

---

---

**Solid mineral fuels — Determination  
of carbonate carbon content —  
Gravimetric method**

*Combustibles minéraux solides — Dosage du carbone sous forme  
de carbonate — Méthode gravimétrique*



Reference number  
ISO 925:1997(E)

## Contents

|   | Page              |
|---|-------------------|
| Foreword  | iii               |
| 1 Scope   | 1                 |
| 2 Normative references  | 1                 |
| 3 Principle   | 1                 |
| 4 Reagents  | 1                 |
| 5 Apparatus   | 2                 |
| 6 Preparation of the test sample  | 2                 |
| 7 Procedure   | 2                 |
| 8 Expression of results   | 4                 |
| 9 Precision   | 4                 |
| 10 Test report  | 4                 |
| Annex A (informative) Derivation of factors used in calculations in this International Standard | Inside back cover |
| Figure 1 — A suitable assembly of the apparatus   | 3                 |
| Table 1 — Precision as carbonate carbon content   | 4                 |
| Table 2 — Precision as carbon dioxide content   | 4                 |
| Table A.1   | Inside back cover |

**Descriptors:** Fossil fuels, solid fuels, carbonates, chemical analysis, determination of content, carbon, gravimetric analysis.

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 925 was prepared by Technical Committee ISO/TC 27, *Solid mineral fuels*, Subcommittee SC 5, *Methods of analysis*.

This third edition cancels and replaces the second edition (ISO 925:1980), which has been technically revised.

Annex A of this International Standard is for information only.





## 1 Scope

This International Standard specifies a gravimetric method of determining the carbon in the mineral carbonates associated with solid mineral fuels.

NOTE The result obtained will include any carbon from atmospheric carbon dioxide absorbed by the fuel.

## 2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 331:1983, *Coal — Determination of moisture in the analysis sample — Direct gravimetric method.*

ISO 687:1974, *Coke — Determination of moisture in the analysis sample.*

ISO 1015:1992, *Brown coals and lignites — Determination of moisture content — Direct volumetric method.*

ISO 1170:1977, *Coal and coke — Calculation of analyses to different bases.*

ISO 1988:1975, *Hard coal — Sampling.*

ISO 2309:1980, *Coke — Sampling.*

ISO 5068:1983, *Brown coals and lignites — Determination of moisture content — Indirect gravimetric method.*

ISO 5069-2:1983, *Brown coals and lignites — Principles of sampling — Part 2: Sample preparation for determination of moisture content and for general analysis.*

ISO 9411-1:1994, *Solid mineral fuels — Mechanical sampling from moving streams — Part 1: Coal.*

ISO 9411-2:1993, *Solid mineral fuels — Mechanical sampling from moving streams — Part 2: Coke.*

## 3 Principle

A known mass of sample is treated with hydrochloric acid, which reacts with the carbonates present to liberate carbon dioxide. The carbon dioxide resulting from the decomposition of the carbonates is absorbed and weighed.

## 4 Reagents

**WARNING — Care should be exercised when handling reagents, many of which are toxic and corrosive.**

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and only distilled water, or water of equivalent purity.

NOTE Distilled water may be freed from carbon dioxide by boiling gently for 15 min.

4.1 *Hydrochloric acid*, approximately 3 mol/l.

4.2 *Hydrogen sulfide absorbent*

Any of the following:

a) copper(II) phosphate, granular, particle size 1,2 mm to 0,7 mm;

NOTE 1 Copper(II) phosphate granules may be prepared as follows:

Mix copper(II) phosphate powdered reagent to a stiff paste with 1 % starch solution. Press through a sheet of metal, perforated with apertures of approximately 1 mm diameter. Dry the extruded material at 110 °C. Sieve to recover the desired size fraction.

b) copper(II) sulfate, deposited on a supporting base of ground pumice;

NOTE 2 A suitable absorbent, based on copper(II) sulfate, may be prepared as follows:

Prepare pumice by crushing and sieving to obtain the 2,8 mm to 0,7 mm fraction. Transfer approximately 60 g of the prepared pumice to an evaporating basin, covering with a saturated solution of copper(II) sulfate, evaporate to dryness with constant stirring, and heat at 150 °C to 160 °C for 3 h to 4 h. Cool in a desiccator and store in a glass-stoppered bottle.

c) silver sulfate, granular.

4.3 *Magnesium perchlorate*, anhydrous, particle size 1,2 mm to 0,7 mm.

**WARNING — Due regard must be taken of local regulations when disposing of exhausted magnesium perchlorate. It is essential that regeneration of magnesium perchlorate is not attempted, owing to the risk of explosion.**

4.4 *Sodium hydroxide*, on an inert base, preferably of coarse grading, for example 1,7 mm to 1,2 mm, and preferably of the self-indicating type.

4.5 *Wetting agent*, suitable for use in acid solution.

NOTE A liquid wetting agent at a concentration of 100 ml/l or ethanol [95 % (V/V)] are suitable.

4.6 *Check test reagent*

Either of the following:

a) anhydrous sodium carbonate;

b) anhydrous calcium carbonate.

## 5 Apparatus

**5.1 Analytical balance**, capable of weighing to the nearest 0,1 mg.

**5.2 Graduated glassware**, conforming to the requirements for Grade A in the International Standards prepared by ISO/TC 48, *Laboratory glassware and related apparatus*.

**5.3 Purification tube**, consisting of an absorption tube<sup>1)</sup> containing sodium hydroxide on an inert base (4.4).

**5.4 Reaction flask assembly**, comprising a 300 ml round-bottomed flask fitted with a tap funnel, a double-surface condenser and a bulb tube.

**5.5 Absorption train**, consisting of three absorption tubes a), b) and c)<sup>1)</sup> packed respectively as follows:

- a) magnesium perchlorate (4.2) to dry the gas;
- b) hydrogen sulfide absorbent (4.2) followed by a protective layer of magnesium perchlorate (4.3). The connection from this tube to tube c) shall be fitted at its outlet end with a stopcock or other means of closure;
- c) sodium hydroxide on an inert base (4.4), to absorb carbon dioxide generated in the reaction flask, followed by a protective layer of magnesium perchlorate (4.3) to absorb water produced in the reaction between carbon dioxide and sodium hydroxide. This tube shall be fitted with stopcocks or other means of closure at the inlet and outlet ends.

### 5.6 Air circulation equipment

A suction pump, capable of drawing air at a rate of 50 ml/min through the apparatus, connected through a flowmeter to a tee-piece fitted with a stopcock (the air vent).

### 5.7 Heating source

, for the reaction flask.

Either an electric heating mantle to accommodate a 300 ml flask or a small gas burner.

An example of a suitable assembly of the apparatus is illustrated in Figure 1.

## 6 Preparation of the test sample

The test sample is the general analysis test sample prepared in accordance with ISO 1988, ISO 2309, ISO 5069-2, ISO 9411-1 or ISO 9411-2 as appropriate. Ensure that the moisture content of the sample is in equilibrium with the laboratory atmosphere, exposing it, if necessary, in a thin layer for the minimum time required to achieve equilibrium.

Before commencing the determination, thoroughly mix the equilibrated test sample for at least one minute, preferably by mechanical means.

If the results are to be calculated other than on an "air-dried" basis (see clause 8), then, after weighing the test portion (see 7.2), determine the moisture content using a further portion of the test sample by the method described in ISO 331, ISO 687, ISO 1015 or ISO 5068, as appropriate.

## 7 Procedure

### 7.1 Check test

Check the air-tightness of the apparatus and condition of the reagents by running a test according to the procedure described in 7.2, but using approximately 60 mg of the check test reagent (4.6), weighed to the nearest 0,1 mg, instead of the test sample.

Calculate the theoretical mass of carbon dioxide (see A.2), expected to be liberated from the check test portion, and compare it with the measured value. The test is satisfactory if the measured value is within 10 % of the theoretical value; otherwise check the apparatus carefully to seal any leaks and/or replace the reagents. Re-test until a satisfactory result is obtained.

Carry out check tests after initially setting up the apparatus, after having made any changes to it or to the reagents, and before making a determination or series of determinations.

### 7.2 Determination

#### 7.2.1 Preparation

Weigh accurately, to the nearest 0,01 g, 5 g of the sample into the reaction flask and add 5 drops of the wetting agent (4.5) and 100 ml of water. Close the flask by means of a rubber stopper and shake vigorously to wet the sample. Remove the stopper and wash any sample adhering to it back into the flask. Assemble the apparatus as shown in Figure 1, with the air vent closed.

**NOTE** For fuels containing more than 0,5 % carbonate carbon, the sample mass may be reduced pro-rata, to a minimum of 0,5 g.

<sup>1)</sup> Absorption tubes may be U-tubes or Midvale tubes (which reduce back-pressure and hence, risk of leakage). The tops of the reagent columns should be covered with a layer of glass wool to guard against entrainment of any fine particles in the circulating air.

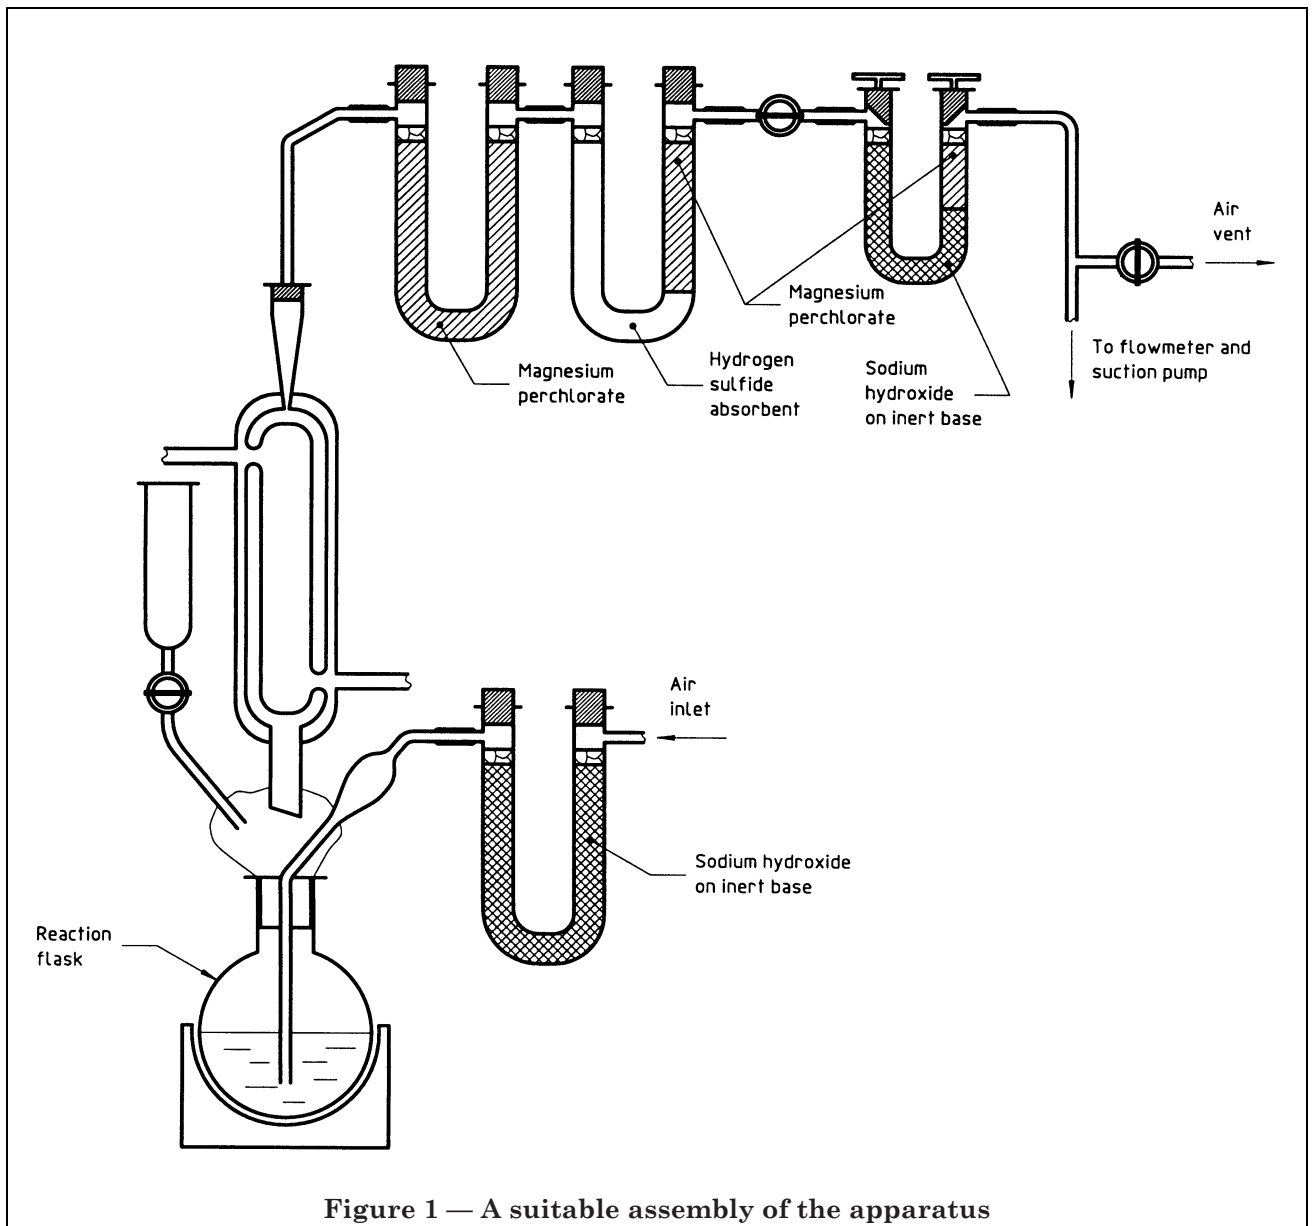


Figure 1 — A suitable assembly of the apparatus

### 7.2.2 Conditioning

Draw air through the apparatus at a rate of 50 ml/min for 10 min. Stop the circulation of air and close the ends of the carbon dioxide absorption tube and the outlet end of the hydrogen sulfide absorption tube connected to it. Remove the carbon dioxide absorption tube and wipe it with a clean, dry, lint-free cloth.

NOTE 1 Under certain conditions of humidity, wiping the absorbers with a cloth may induce a static charge, which, if significant, could affect the weighing. Consideration should therefore be given to employing static eliminators.

Allow the tube to cool to the balance room temperature and weigh it at 10 min intervals until constant weight is obtained, i.e. two successive weighings do not differ by more than 1 mg.

NOTE 2 Tubes used for the absorption of carbon dioxide, particularly Midvale tubes, cool slowly and up to 60 min should be allowed before weighing. When not connected to the apparatus, the tubes should be protected from atmospheric contamination by closing the taps and fitting guard seals of plugged rubber tubing to the open limbs. It is usual to weigh the absorption tubes without guard seals, after wiping.

### 7.2.3 Reaction and completion

Reconnect the absorption tube to the apparatus and open the stopcocks or other closures in the absorption train. Place 25 ml of the hydrochloric acid (4.1) in the tap funnel, open the air vent and admit the acid to the reaction flask. Close the air vent and draw air through the system at a rate of about 50 ml/min. Raise the temperature of the liquid in the reaction flask slowly so that it boils after about 15 min. Continue boiling for a further 30 min, the rate of boiling being adjusted so that the condenser is not overloaded. Turn off the heating source, stop the circulation of air, remove the absorption tube, wipe clean and weigh as before (see 7.2.2).

## 8 Expression of results

Results may be expressed in terms of carbonate carbon content or carbon dioxide content, as appropriate, as follows.

The carbonate carbon content of the sample  $W_C$ , as analyzed, expressed as a percentage by mass, is given by the formula

$$W_C = \frac{27,29 \times m_2}{m_1}$$

and the carbon dioxide content of the sample,  $W_{CO_2}$ , as analyzed, expressed as a percentage by mass, is given by the formula

$$W_{CO_2} = \frac{100 \times m_2}{m_1}$$

where

$m_1$  is the mass, in grams, of the test portion;

$m_2$  is the increase in mass, in grams, of the absorption tube.

Report the results as the mean of duplicate determinations, to the nearest 0,01 %.

The results of the determination described in this International Standard are reported on the "air-dried" basis. Calculation of results to other bases is dealt with in ISO 1170.

## 9 Precision

### 9.1 Repeatability limit

The results of duplicate determinations, carried out at different times within a short interval, in the same laboratory, by the same operator, with the same apparatus, on representative portions taken from the same analysis sample, should not differ by more than the values shown in Table 1 or Table 2, as appropriate.

### 9.2 Reproducibility critical difference

The means of the results of duplicate determinations, carried out in each of two laboratories, on representative portions taken from the same sample after the last stage of sample preparation, should not differ by more than the values shown in Table 1 or Table 2, as appropriate.

## 10 Test report

The test report shall include the following particulars:

- reference to this International Standard;
- an identification of the sample tested;
- the results and the method of expression used;
- any unusual features noted during the determination;
- any operation not included in this International Standard, or regarded as optional;
- the date of the test.

**Table 1 — Precision as carbonate carbon content**

| Carbonate carbon | Maximum acceptable differences between results<br>(calculated to the same moisture content) |   |
|------------------|---|---|
|                  | Same laboratory<br>(repeatability)  | Different laboratories<br>(reproducibility) |
| Up to 0,4 %      | 0,02 % absolute   | 0,04 % absolute                             |
| 0,4 % and over   | 5 % relative  | 10 % relative                               |

**Table 2 — Precision as carbon dioxide content**

| Carbon dioxide | Maximum acceptable differences between results<br>(calculated to the same moisture content) |   |
|----------------|---|---|
|                | Same laboratory<br>(repeatability)  | Different laboratories<br>(reproducibility) |
| Up to 1 %      | 0,05 % absolute   | 0,1 % absolute                              |
| 1 % and over   | 5 % relative  | 10 % relative                               |

**Annex A (informative)****Derivation of factors used in calculations in this International Standard****A.1 General**

In this annex, relative atomic masses and relative molecular masses are represented by the chemical formulae in square brackets. The relative atomic masses given in Table A.1 were used in the calculations.

**Table A.1**

| Element  | Symbol | Relative atomic mass |
|----------|--------|----------------------|
| Hydrogen | H      | 1,008                |
| Carbon   | C      | 12,011               |
| Oxygen   | O      | 15,999               |
| Sodium   | Na     | 22,990               |
| Calcium  | Ca     | 40,078               |

**A.2 Check test**

The theoretical mass of carbon dioxide,  $m_{\text{CO}_2}$ , liberated from a given mass,  $m_{\text{Na}}$ , of the sodium carbonate check test reagent is given by the formula:

$$m_{\text{CO}_2} = \frac{[\text{CO}_2]}{[\text{Na}_2\text{CO}_3]} \times m_{\text{Na}} = \frac{44,009}{105,998} \times m_{\text{Na}} = 0,415\ 2\ m_{\text{Na}}$$

The theoretical mass of carbon dioxide,  $m_{\text{CO}_2}$ , liberated from a given mass,  $m_{\text{Ca}}$ , of the calcium carbonate check test reagent is given by the formula:

$$m_{\text{CO}_2} = \frac{[\text{CO}_2]}{[\text{CaCO}_3]} \times m_{\text{Ca}} = \frac{44,009}{100,086} \times m_{\text{Ca}} = 0,439\ 7\ m_{\text{Ca}}$$

**A.3 Determination**

The percentage, by mass, of carbonate carbon,  $W_{\text{C}}$ , in the sample is given by the formula:

$$W_{\text{C}} = \frac{[\text{C}] \times m_2 \times 100}{[\text{CO}_2] \times m_1} = \frac{27,29 \times m_2}{m_1}$$

where

$m_1$  is the mass, in grams, of the test portion;

$m_2$  is the increase in mass, in grams, of the absorption tube.

---

---

## **BSI — British Standards Institution**

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

### **Revisions**

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.  
Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

### **Buying standards**

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

### **Information on standards**

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.  
Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.  
Tel: 020 8996 7002. Fax: 020 8996 7001.

### **Copyright**

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager.  
Tel: 020 8996 7070.