

Methods for

Measurement of air pollution —

**Part 6: Sampling equipment used for
the determination of gaseous sulphur
compounds in ambient air**

[ISO title: Air quality — Determination of gaseous sulphur
compounds in ambient air — Sampling equipment]

UDC 551.510.42:614.72:551.508.95:546.22-13

Cooperating organizations

The Environment and Pollution Standards Committee, under whose direction this British Standard was prepared, consists of representatives from the following:

Association of County Councils
 British Gas Corporation*
 British Industrial Measuring and Control Apparatus Manufacturers' Association (BEAMA)
 British Paper and Board Industry Federation (PIF)
 British Railways Board
 British Steel Corporation*
 Chemical Industries Association
 Confederation of British Industry
 Consumer Standards Advisory Committee of BSI
 Council of Engineering Institutions
 Council of Environmental Conservation
 Department of Industry (Laboratory of the Government Chemist)*
 Department of Industry (Warren Spring Laboratory)*
 Department of the Environment (Water Directorate)
 Department of Transport
 Electricity Supply Industry in England and Wales*
 Engineering Equipment Users' Association
 Greater London Council
 Health and Safety Executive*
 Institute of Petroleum*
 Medical Research Council
 Ministry of Agriculture, Fisheries and Food
 National Coal Board*
 National Water Council
 Royal Society of Chemistry
 Scottish Office
 Trades Union Congress

The organizations marked with an asterisk in the above list, together with the following, were directly represented on the Technical Committee entrusted with the preparation of this British Standard:

Cement Makers' Federation
 Department of Health and Social Security
 Institution of Environmental Health Officers
 Institution of Gas Engineers
 Lead Development Association
 National Industrial Fuel Efficiency Service
 National Society for Clean Air

This British Standard, having been prepared under the direction of the Environment and Pollution Standards Committee, was published under the authority of the Board of BSI and comes into effect on 31 January 1983

© BSI 08-1999

The following BSI references relate to the work on this standard:
 Committee reference EPC/35
 Draft for comment 77/52934 DC

ISBN 0 580 13121 1

Amendments issued since publication

Amd. No.	Date of issue	Comments

Contents

	Page
Cooperating organizations	Inside front cover
National foreword	ii
<hr/>	
0 Introduction	1
1 Scope	1
2 Field of application	1
3 Definition	1
4 Principle	1
5 Equipment	1
6 Installation	4
<hr/>	
Figure 1 — Block diagram of sampling equipment	2
Figure 2 — Air intake with protecting funnel	2
<hr/>	
Publications referred to	Inside back cover
<hr/>	

National foreword

This Part of this British Standard, which has been prepared under the direction of the Environment and Pollution Standards Committee, is identical with ISO 4219:1979 “*Air quality — Determination of gaseous sulphur compounds in ambient air — Sampling equipment*”. The International Standard was prepared by Technical Committee 146, Air quality, and published by the International Organization for Standardization (ISO) as a result of discussion in which the UK participated.

This Part of this British Standard is one of a series relating to air quality arising from UK participation in the work of ISO/TC 146. Methods for the determination of particular constituents of ambient air will be published as further Parts of this standard. Topics relating to air quality characteristics will be published as Parts of BS 6069 “*Methods for characterization of air quality*”.

Terminology and conventions. The text of the International Standard has been approved as suitable for publication as a British Standard without deviation. Some terminology and certain conventions are not identical with those used in British Standards; attention is especially drawn to the following.

The comma has been used as a decimal marker. It is current practice in British Standards to use a full point on the baseline as the decimal marker.

Wherever the words “International Standard” appear, referring to this standard, they should be read as “British Standard”.

Cross-references

International Standard	Corresponding British Standard
ISO 4221:1980	BS 1747 <i>Methods for measurement of air pollution</i> Part 7:1982 <i>Determination of mass concentration of sulphur dioxide in ambient air: Thorin spectrophotometric method</i> (Identical)

ISO 4220, to which reference is made in clauses **0**, **2** and **3**, is still in course of preparation. When it is published, consideration will be given to publishing it as a dual numbered British Standard.

Additional information. 3 Definition. The definition for “gaseous sulphur compounds” is liable to misinterpretation and the following has been reported to ISO in a proposal to amend the text of the International Standard.

“gaseous sulphur compounds: Sulphur dioxide and other gaseous sulphur compounds, and, in addition, water-soluble acidic gases determined according to the method in ISO 4220.”

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, pages 1 to 4, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

0 Introduction

The determination of gaseous sulphur compounds in ambient atmospheres requires as a first step the collection of a sample of air and the absorption of the constituents to be determined in a suitable liquid medium. The specific absorption media and some of the sampling conditions may vary according to the methods. This International Standard provides details of the equipment required thus obviating the necessity for specification in detail of the equipment in each of the separate International Standards concerned with methods of determination of gaseous sulphur compounds. The method of sampling is covered in ISO 4220 and 4221.

1 Scope

This International Standard specifies general requirements for the equipment for the sampling of ambient air in order to determine gaseous sulphur compounds, particularly sulphur dioxide.

2 Field of application

This International Standard is applicable to ambient air. It is applicable to the sampling of air for sulphur dioxide and other gaseous sulphur compounds as defined in clause 3.

It is primarily intended to be used in conjunction with the following International Standards:¹⁾

ISO 4220, *Air quality — Determination of a gaseous acid pollution index — Titrimetric method with indicator or potentiometric end-point detection.*

ISO 4221, *Air quality — Determination of mass concentration of sulphur dioxide in ambient air — Thorin spectrophotometric method.*

which specify supplementary details relating to the sampling equipment, the absorbing solution and the sampling procedure.

The sampling equipment specified may also be used for determinations other than gaseous sulphur compounds.

3 Definition

gaseous sulphur compounds

sulphur dioxide, other gaseous sulphur compounds and water-soluble acidic gases determined according to the method of ISO 4220

4 Principle

Drawing of ambient air through an absorber to trap the gaseous sulphur compounds being determined. Under certain circumstances, detailed in the relevant International Standard, filtration of the air to remove interfering particulates.

5 Equipment

Because gaseous sulphur compounds are very reactive, the use of the correct materials for all parts of the sampling equipment coming into contact with the air containing these compounds is essential.

Materials used shall not absorb any of the constituents to be determined and shall not react with them to produce a reaction product that might interfere with subsequent determination or to reduce the concentration of the constituents.


The equipment shall consist essentially of the following components, each of which is separately described in 5.1 to 5.7:

- air intake;
- connecting tubing;
- particulate filter and filter holder;
- absorber;
- protection filter;

¹⁾ An International Standard specifying a tetrachloromercurate (TCM) pararosaniline spectrophotometric method for the determination of the mass concentration of sulphur dioxide in ambient air is in preparation.


- sampling pump;
- gas meter or air-flow regulator.

A schematic layout of a typical assembly system is shown in Figure 1:

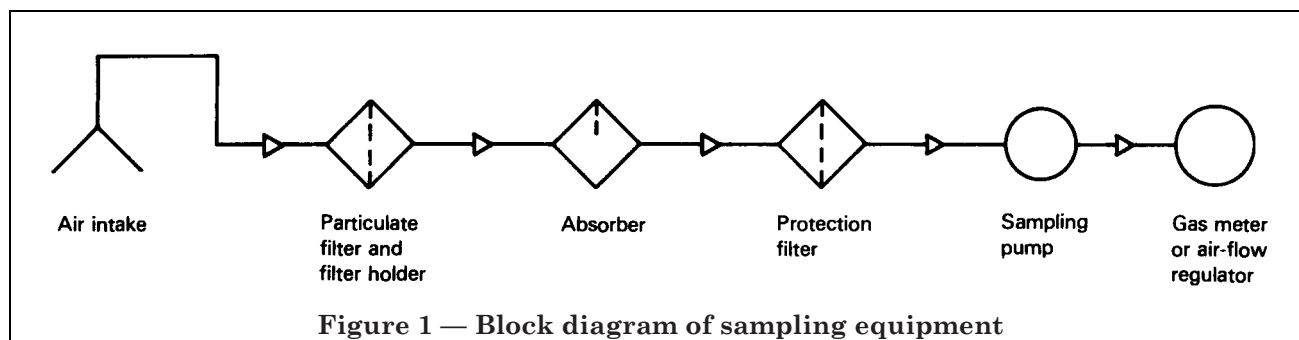

5.1 Air intake

No particular design of air intake is required for this International Standard concerning determination of gaseous sulphur compounds only. If the air intake may be exposed to precipitation, an inverted funnel may be used as protection, as shown in Figure 2.

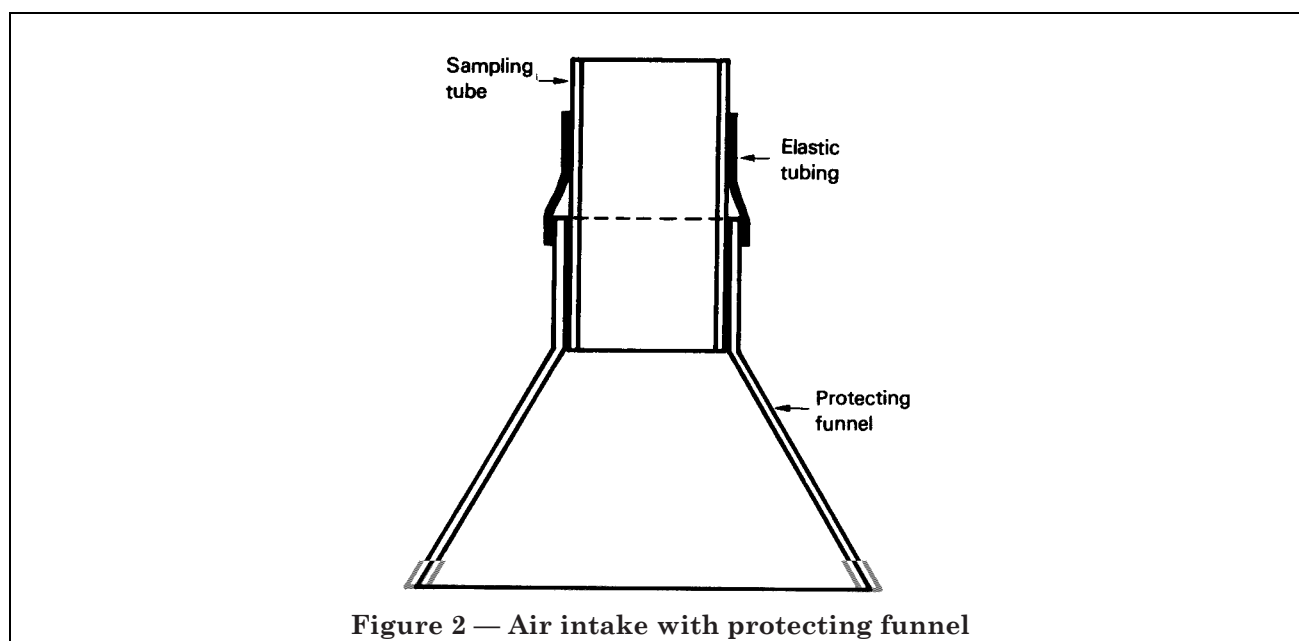

If it is intended to carry out other determinations, e.g. concentration of black smoke with the same equipment (see clause 2), the air must be drawn in through an air intake of appropriate diameter.

5.2 Connecting tubing

5.2.1 Dimensions

The internal diameter of the tubing shall be 6 to 8 mm and the internal surface shall be smooth.

5.2.2 *Material*

In addition to the general requirements for materials, plastics materials used shall be protected from actinic activity and preferably should be covered with a material having a low thermal conductivity. All tubing shall be airtight. Regular cleaning of the tubing is recommended. The following materials, in order of preference according to descending effectiveness, may be used:

- a) Polytetrafluorethylene (PTFE). Although chemically inert, PTFE is not flexible and difficulty may be experienced in making connections. Connections with PTFE can be made successfully using connectors which are available in PTFE. In addition, in view of the inflexibility of PTFE, there is no need to use PTFE downstream of the sample absorber. Rubber vacuum hose should be the preferred material since it is flexible, makes good seals and will not affect the sample because the components of interest have already been removed.
- b) Glass. Glass is fragile. It is suggested that connections to components be made using butt joints with flexible PVC tubing.
- c) Polypropylene (polyethylene).

Agents used for cleaning tubing shall be sulphur free.

5.3 *Particulate filter*

The assembly shall be airtight in use; hence, an appropriate clamping device shall be used together with an annular seal. Air shall be drawn upwards through the filter.

5.3.1 *Filter material*

The material of the filter shall be chemically inert with respect to sulphur compounds, and shall not be hygroscopic.

The filter shall possess high efficiency (99 %) for particles above 0,3 μm .

If the filter is being used simply to remove particulate matter (which interferes with some methods of analysis), a suitable filter is a pad of polystyrene fibres²⁾. This filter has excellent efficiency and low pressure drop, and the material is inert. Other kinds of inert filter can also be used.

The use of glass fibre filter material is not recommended as it is too reactive (see first paragraph).

NOTE Under conditions of high humidity, the particulate filter may become damp and thus absorb some sulphur compounds from the air passing through it. These conditions should be noted in the test report. The heating of the filter under such conditions is not recommended due to the possibility of side reactions. However, under some climatic conditions, it is found necessary to warm the filter above the dew point.

5.3.2 *Filter holder*

The filter holder shall be made from inert material, for an example an inert form of PVC.

5.4 *Absorber*

The design of the absorption bottle, in which the absorption solution is contained, is dependent on the particular analysis to be employed and on the sampling flow rate. The relevant International Standards shall be consulted.

5.5 *Protection filter*

If a liquid absorbent is employed, it may be necessary to insert a trap between the absorption bottle and the gas meter (or the air-flow regulator) to protect the latter from absorbing solution droplets and/or harmful gases. The design of the trap is not critical, provided that air is not allowed to enter the system through leakage (it will normally be under slight suction).

5.6 *Gas meter or air-flow regulator*

In order to calculate the relevant concentration, the volume of air sampled must be known. The volume is best measured by an integrating method, for example by using a dry-gas meter. This shall be able to record the volume of sampled air to a sufficient accuracy at the flow rate used. A flow-regulating system based on the use of a critical orifice may alternatively be used. The flow shall then be checked at the beginning and end of the sampling period at the air intake with a device such as a variable-area flow meter to ensure that the flow rate has not changed because of partial plugging of the orifice.

Calibration of these meters or orifices may be carried out by comparison with a laboratory wet-gas meter which has itself been subjected to primary calibration within the preceding 2 years.

²⁾ For example, Microsorban.

5.7 Sampling pump

The most suitable device for sampling is a constant-flow air pump.

The type of pump should preferably be chosen for the intended air flow rate as it is not good practice to control a pump flow rate by voltage variations.

Unless the pump is placed after the gas meter, it shall be leak proof.

6 Installation

Install the equipment in an environment in which it is not exposed to extreme temperatures or to direct sunlight for long periods.

Arrange the air intake (5.1) so that it is at least 1 m from all obstacles, including sampling equipment, and more than 3 m above the nearest large area of horizontal surface. The tubing or funnel shall point vertically downwards.

Take care to avoid placing the air intake anywhere near local sources of pollution, such as a low-level chimney or an exhaust vent.

NOTE The choice of a site which is representative of the relevant concentration in a given geographical area, and the number of sites required for adequate coverage of a given area, will be the subject of other International Standards.

Arrange the connecting tubing (5.2) in such a way that there are no loops in which water may collect and no radii less than 50 mm. The latter condition is particularly important if a black smoke index is being determined with the same equipment.

The total length of tubing between air intake and absorber (5.4) shall be as short as possible and in any case shall be less than 6 m.

Check that all connections between the components of the equipment are airtight.

Publications referred to

See national foreword.

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.
Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.
Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.
Tel: 020 8996 7002. Fax: 020 8996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager.
Tel: 020 8996 7070.